

STANDARD F


Strep A Ag FIA SD BIOSENSOR

STANDARD F Strep Ag FIA test system (Analyzer + Test device) detects group A Streptococcal (Strep A) antigen directly from throat swabs of symptomatic patients or confirmation of presumptive Group A Streptococcal colonies recovered from culture.




Specification	
Intended use	Qualitative detection of Group A Streptococcus antigen in respiratory specimens.
Specimen volume	100 µl
Specimen type	Throat swab
Measurement range	Quantitative result with cut-off index (COI)
Testing time	5 mins (Early detection available)
Storage condition	2 - 30°C / 36 - 86°F

METHOD OF SAMPLE COLLECTION




Throat Swab

STANDARD TEST MODE

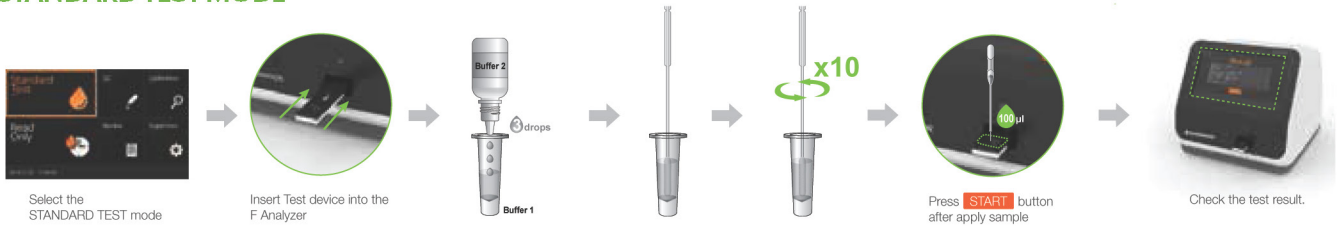

READ ONLY MODE

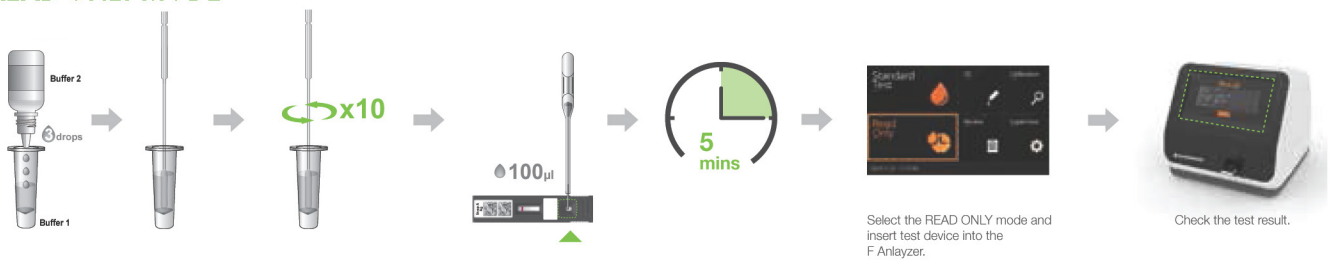

TEST PERFORMANCE

Reference	Sensitivity	Specificity
Bacterial Culture	93.3% (28/30)	95% (38/40)

ORDERING INFORMATION

Category	Product	Pack Size
Respiratory	STANDARD F Strep A Ag	25 Test
	STANDARD F Strep A Ag Control	Pos x 10 / Neg x 10